

# Comparison between High-Performance Liquid Chromatography and Enzyme-linked Immunosorbent Assay for the Determination of 8-Hydroxy-2'-deoxyguanosine in Human Urine<sup>1</sup>

Kayoko Shimoi,<sup>2</sup> Hiroshi Kasai, Naoko Yokota, Shinya Toyokuni, and Naohide Kinai

Institute for Environmental Sciences [K. S.], and Department of Food and Nutritional Sciences, Graduate School of Nutritional and Environmental Sciences [N. Y., N. K.], University of Shizuoka, Shizuoka 422-8526; Department of Environmental Oncology, University of Occupational and Environmental Health, Kitakyushu 807-8555 [H. K.]; and Department of Pathology and Biology of Diseases, Graduate School of Medicine, Kyoto University, Kyoto 606-8501 [S. T.], Japan

## Abstract

**8-Hydroxy-2'-deoxyguanosine (8-OH-dG), which has been regarded as a potential marker of oxidative DNA damage induced by reactive oxygen species, was measured in human urine by a commercial ELISA using a monoclonal antibody N45.1 and by high-performance liquid chromatography (HPLC) coupled to an electrochemical detector (HPLC-ECD) to evaluate whether the ELISA system is applicable to human monitoring studies. The urine samples were collected from 120 healthy men ages 18–58 in a steel-manufacturing company. A good correlation ( $r = 0.833$ ;  $P < 0.0001$ ) was observed between the two methods on HPLC-purified 8-OH-dG fractions from 23 urine samples. The mean value ( $\pm$ SD) of 8-OH-dG ( $\mu$ g/g creatinine) was 5.47 ( $\pm$ 2.97) by HPLC-ECD assay and 5.50 ( $\pm$ 2.36) by ELISA. However, the correlation ( $r$ ) between the two methods on 120 original urine samples was 0.460 [ $P < 0.001$ ; mean value ( $\pm$ SD) of 8-OH-dG ( $\mu$ g/g creatinine) was 4.46 ( $\pm$ 2.03) by the HPLC assay and 9.33 ( $\pm$ 3.23) by ELISA]. ELISA estimates were about 2-fold higher than the HPLC estimates on original urine. For an unknown reason, 10% of the urine samples showed more than a 4-fold increase in value by ELISA. It is suggested that the ELISA system is applicable for comparative human monitoring studies. Prepurification of samples is required to determine the absolute value of 8-OH-dG in individual urine samples by ELISA.**

## Introduction

ROS<sup>3</sup> are endogenously generated in cells and may be involved in aging and the development of diseases such as cancer and

diabetes. 8-OH-dG has been regarded as a potential marker of oxidative DNA damage induced by ROS (1) and has been analyzed as a marker of cellular oxidative stress relevant to carcinogenesis (2). 8-OH-dG was increased in the DNA of target organs after treatment with carcinogens that generate ROS in animal experiments (2). In humans, higher levels of 8-OH-dG were observed in the lungs of smokers (3), the liver of chronic hepatitis patients (4), lymphocytes from cancer patients during radiotherapy (5), and mononuclear cells from diabetic patients (6).

The level of urinary 8-OH-dG has been reported to be higher in cancer patients than in healthy people (7) and higher in smokers than in nonsmokers (8), and to be affected by metabolic rate (9). The urinary 8-OH-dG has been measured by several methods such as liquid chromatography-tandem mass spectrometry (LC-MS-MS; Ref. 10), gas chromatography with mass spectrometric detection (GC-MS; Ref. 11), and HPLC-ECD (12). Recently, a monoclonal antibody specific to 8-OH-dG (N45.1) has been developed and an ELISA has been established for 8-OH-dG determination (13). Urinary 8-OH-dG levels increased in non-small cell carcinoma patients during the course of radiotherapy and small cell carcinoma patients showed higher levels of urinary 8-OH-dG than did controls (14). However, it has been reported that a commercially available ELISA kit using N45.1 monoclonal antibody yields ~8-fold higher results, on average, with a high variation, compared with the HPLC-ECD method (15). It was suggested that there may be cross-reacting substances in urine. Because it is more simple and easier to measure urinary 8-OH-dG by the ELISA method than by HPLC analysis in the aspects of equipment, analyzing time, running cost, and urine sample volume, the number of reports on urinary 8-OH-dG levels determined by ELISA has been on the increase recently. However, there remain methodological problems in urine analysis.

In this study, human urinary excretion of 8-OH-dG was determined by the commercial ELISA method, the ELISA method with HPLC prepurification, and the HPLC-ECD method to evaluate whether the ELISA system is applicable to human monitoring studies.

## Materials and Methods

**Urine Collection.** Urine samples were collected in paper cups from 120 healthy men ages 18–58 in a steel-manufacturing company, who gave their informed consent, in the afternoon (12:45–15:30) during their periodic health examination. Aliquots of each urine sample were stored at  $-80^{\circ}\text{C}$  until the 8-OH-dG analysis.

Received 8/31/01; revised 4/8/02; accepted 4/24/02.

The costs of publication of this article were defrayed in part by the payment of page charges. This article must therefore be hereby marked *advertisement* in accordance with 18 U.S.C. Section 1734 solely to indicate this fact.

<sup>1</sup> Supported by Goto Research Grant from University of Shizuoka.

<sup>2</sup> To whom requests for reprints should be addressed, at Institute for Environmental Sciences, Graduate School of Nutritional and Environmental Sciences, University of Shizuoka, 52-1 Yada, Shizuoka 422-8526, Japan. Phone and Fax: 81-54-264-5787; E-mail: shimoi@smail.u-shizuoka-ken.ac.jp.

<sup>3</sup> The abbreviations used are: ROS, reactive oxygen species; 8-OH-dG, 8-hydroxy-2'-deoxyguanosine; HPLC, high-performance liquid chromatography;

ECD, electrochemical detection; HPLC-ECD, HPLC with ECD; ELISA, enzyme-linked immunosorbent assay.

Table 1 Urinary 8-OH-dG/creatinine levels determined by ELISA and HPLC-ECD

	8-OH-dG/creatinine ( $\mu\text{g/g}$ )			ELISA/HPLC
	Mean $\pm$ SD	Maximum	Minimum	
<i>n</i> = 23				
Original urine				2.63 $\pm$ 2.07
ELISA	10.53 $\pm$ 3.95	19.52	4.35	
HPLC-ECD	5.47 $\pm$ 2.97	11.09	1.20	
8-OHdG purified fraction				1.18 $\pm$ 0.49
ELISA	5.50 $\pm$ 2.36	9.61	2.20	
HPLC-ECD	5.47 $\pm$ 2.97	11.09	1.20	
<i>n</i> = 120				
Original urine				2.43 $\pm$ 1.31
ELISA	9.33 $\pm$ 3.23	19.52	3.93	
HPLC-ECD	4.46 $\pm$ 2.03	11.09	1.20	
<i>n</i> = 27				
Original urine (nonsmoker)				2.21 $\pm$ 0.79
ELISA	8.16 $\pm$ 2.66	14.14	4.35	
HPLC-ECD	4.18 $\pm$ 2.13	10.47	1.52	
<i>n</i> = 76				
Original urine (smoker)				2.57 $\pm$ 1.51
ELISA	9.91 $\pm$ 3.34	19.52	4.90	
HPLC-ECD	4.57 $\pm$ 2.03	11.09	1.20	
<i>n</i> = 21				
Original urine (smoker: more than 26 cigarettes/day)				2.54 $\pm$ 1.99
ELISA	10.81 $\pm$ 3.37	19.52	5.44	
HPLC-ECD	5.19 $\pm$ 2.10	8.99	1.20	

**HPLC Analysis and Fractionation of 8-OH-dG.** HPLC analysis was carried out by the method described previously (16). Briefly, 1.0 ml of each urine sample was defrosted, diluted with 0.5 ml of water, and acidified with 45  $\mu\text{l}$  of acetic acid. The urine solution was centrifuged, and 0.75 ml of the supernatant was automatically injected into the first HPLC column [Shodex Asahipak GS-320HQ 7G (500  $\times$  7.6 mm), 25°C], which has the functions of gel filtration-, reverse phase-, and ion exchange-column fractionation. Elution was performed using 0.1% acetic acid at the flow rate of 1 ml/min. An aliquot (100  $\mu\text{l}$ ) of the fraction containing 8-OH-dG (50–61 min) was automatically injected into the second HPLC column [YMC-Pack ODS-AM. (250  $\times$  4.6 mm), 25°C]. The mobile phase was aqueous methanol (5%) containing 35 mM NaOAc and 12.5 mM citric acid (pH was adjusted to 7.5 by adding 1M NaOH solution). The flow rate was 0.8 ml/min. The HPLC system was equipped with an ECD (Coulchem II, esa; guard cell, 350 mV; channel 1, 300 mV; channel 2, 150 mV) for detection. Quantification of 8-OH-dG was done by measuring the peak areas based on calibration plots of the peak area of standard 8-OH-dG at various concentrations. The accuracy of the measurement estimated from the recovery of an added 8-OH-dG standard was 90–98%.

8-OH-dG fraction (50–61 min) was collected through the first HPLC column as mentioned above, and the solution was evaporated into dryness by a freeze dryer for the ELISA method.

Urinary creatinine was determined by a kit (Creatinine-test, Wako, Osaka).

**ELISA for Urinary 8-OH-dG.** Urine samples were centrifuged at 2000  $\times g$  for 15 min and 50  $\mu\text{l}$  of the supernatant was used for the determination of 8-OH-dG with a commercial ELISA kit (New 8-OHdG check, Japan Institute for the Control of Aging, Fukuroi, Shizuoka). The determination range was 0.5–200 ng/ml. The monoclonal antibody, N45.1, with an es-

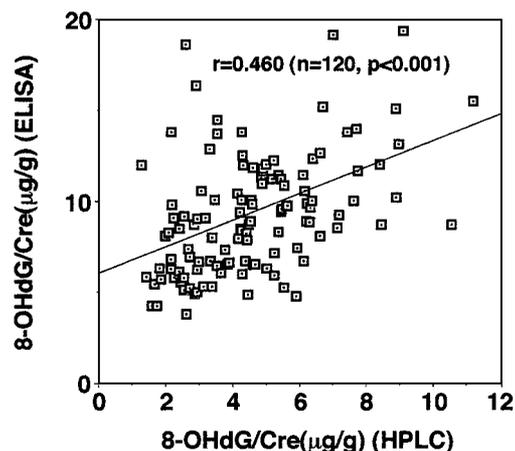


Fig. 1. Correlation between the two methods, HPLC and ELISA, on human urinary 8-OH-dG levels of 120 volunteers (men).

established specificity (13), was used as a primary antibody. The values from each urine sample were calculated based on calibration sigmoid plots of absorbance (492 nm) of standard 8-OH-dG at various concentrations, by fitting a logistic curve using a computer analysis. Day-to-day variation was less than 10%.

**Statistical Analysis.** Data were shown as 8-OH-dG/creatinine ( $\mu\text{g/g}$ ). The correlation between the HPLC and the ELISA estimate was tested by a simple linear regression analysis.

## Results

As shown in Table 1, the mean value (mean  $\pm$  SD) of 8-OH-dG in 120 urine samples was 4.46  $\pm$  2.03  $\mu\text{g/g}$  creatinine by HPLC analysis and 9.33  $\pm$  3.23  $\mu\text{g/g}$  creatinine by the ELISA method,

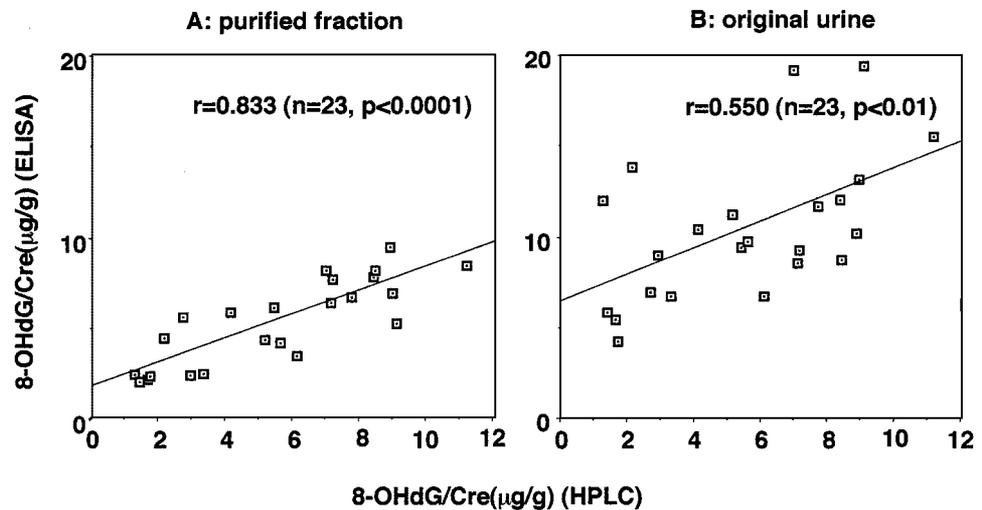


Fig. 2. Correlation between the two methods, HPLC and ELISA, on 8-OH-dG level of 23 human original urine samples (B) and their 8-OH-dG purified fractions (A).

the ELISA estimate being  $\sim 2$ -fold higher than the HPLC estimate. The increase of the mean value of urinary 8-OH-dG in smokers, especially in heavy smokers (more than 26 cigarettes/day), was shown by both methods. The correlation between the two methods was 0.460 ( $P < 0.001$ ; Fig. 1). The ratio of ELISA:HPLC values ranged from 0.84 to 10.08 with a mean of  $2.43 \pm 1.31$  (mean  $\pm$  SD). Ten % of the urine samples showed a  $>4$ -fold higher ratio.

However, a good correlation ( $r = 0.833$ ;  $P < 0.0001$ ) was observed between the two methods on HPLC-purified 8-OH-dG fractions from 23 urine samples (Fig. 2A). The mean value of 8-OH-dG in the purified fraction from 23 urine samples was  $5.47 \pm 2.97$   $\mu\text{g/g}$  creatinine (mean  $\pm$  SD) by HPLC analysis and  $5.50 \pm 2.36$   $\mu\text{g/g}$  creatinine by the ELISA method. The interindividual variation by each method was 9.2-fold (1.20–11.09  $\mu\text{g/g}$  creatinine) and 4.4-fold (2.20–9.61  $\mu\text{g/g}$  creatinine), respectively. The ELISA estimate was almost the same as the HPLC estimate (Fig. 2A). The mean value of 8-OH-dG in 23 original urine samples was  $5.47 \pm 2.97$   $\mu\text{g/g}$  creatinine (mean  $\pm$  SD) by HPLC analysis and  $10.53 \pm 3.95$   $\mu\text{g/g}$  creatinine (mean  $\pm$  SD) by the ELISA method, respectively. The interindividual variation was  $\sim 9.2$  fold (1.20–11.09  $\mu\text{g/g}$  creatinine) by the HPLC analysis and  $\sim 4.4$ -fold (4.35–19.52  $\mu\text{g/g}$  creatinine) by the ELISA method. The ELISA estimate was about 2-fold higher than the HPLC estimate (Table 1). The correlation between the two methods was 0.550 ( $P < 0.01$ ; Fig. 2B).

## Discussion

In this study, the ELISA estimate was similar to the HPLC estimate on purified 8-OH-dG fractions from 23 urine samples. A good correlation ( $r = 0.833$ ;  $P < 0.0001$ ) was observed between the two estimates. It has been reported that the mean value of 8-OH-dG in human urine samples determined by HPLC-ECD (this study), HPLC-ECD (another group; Ref. 17), gas chromatography with mass spectrometric detection (11), and HPLC-ELISA (this study) was  $5.47 \pm 2.97$  (mean  $\pm$  SD), 3.68–3.96, 3.33–3.95, and  $5.50 \pm 2.36$  (mean  $\pm$  SD)  $\mu\text{g/g}$  creatinine, respectively. These results indicate that the monoclonal antibody N45.1 used for a commercial ELISA kit is quite specific for 8-OH-dG.

However, the ELISA estimate on 120 original urine samples ( $9.33 \pm 3.23$   $\mu\text{g/g}$  creatinine) was  $\sim 2$ -fold higher than the

HPLC estimate ( $4.46 \pm 2.03$   $\mu\text{g/g}$  creatinine). A lower correlation was observed between the two estimates compared with the values on the purified 8-OH-dG fractions. Ten % of urine samples showed a high ratio of ELISA-estimates:HPLC-estimates ( $>4$ -fold). These results suggest that the monoclonal antibody N45.1 used for a commercial ELISA kit is not sufficiently specific to detect 8-OH-dG in urine without prior HPLC purification and that crude urine samples contain cross-reacting substances, modified forms of 8-OH-dG, other structurally related compounds, or inhibitors for competition with the N45.1 antibody. There is a possibility that oligonucleotides, as a result of nucleotide excision repair, and glucuronides/sulfates, as a result of metabolic conjugation, are excreted into the urine. Because it has been reported that this antibody, N45.1, recognizes both the modified base and deoxyribose structure (13), N45.1 may react with modified forms of 8-OH-dG or mimicking substances. The reason for the high ELISA estimates remains unknown.

The urinary 8-OH-dG level obtained by ELISA in crude urine in this study was  $9.33 \pm 3.23$   $\mu\text{g/g}$  creatinine. Because it was 17.1 (12) and  $19.4 \pm 8.5$  (14)  $\mu\text{g/g}$  creatinine in the previous reports, the new kit used in this study appears to be somewhat more accurate. It should be noted that the urinary 8-OH-dG level was  $\sim 2$ -fold higher and that 10% of the urine samples showed a very high value by the ELISA method. The results shown in this study suggest that the ELISA system is applicable for comparative human monitoring studies, although HPLC prepurification of samples is required to determine the absolute value of 8-OH-dG in individual urine samples by ELISA.

## References

- Shigenaga, M. K., Aboujaoude, E. N., Chen, Q., and Ames, B. N. Assays of oxidative DNA damage biomarkers 8-oxo-2'-deoxyguanosine and 8-oxoguanine in nuclear DNA and biological fluids by high-performance liquid chromatography with electrochemical detection. *Methods Enzymol.*, 234: 16–33, 1994.
- Kasai, H. Analysis of a form of oxidative DNA damage, 8-hydroxy-2'-deoxyguanosine, as a marker of cellular oxidative stress during carcinogenesis. *Mutat. Res.*, 387: 147–163, 1997.
- Asami, S., Manabe, H., Miyake, J., Tsurudome, Y., Hirano, T., Yamaguchi, R., Itoh, H., and Kasai, H. Cigarette smoking induces an increase in oxidative DNA damage, 8-hydroxydeoxyguanosine, in a central site of the human lung. *Carcinogenesis (Lond.)*, 18: 1763–1766, 1997.
- Shimoda, R., Nagashima, M., Sakamoto, M., Yamaguchi, N., Hirohashi, S., Yokota J., and Kasai, H. Increased formation of oxidative DNA damage, 8-

hydroxydeoxyguanosine, in human livers with chronic hepatitis. *Cancer Res.*, *54*: 3171–3172, 1994.

5. Bialkowski, K., Kowara, R., Windorbska, W., and Olinski, R. 8-Oxo-2'-deoxyguanosine level in lymphocytes DNA of cancer patients undergoing radiotherapy. *Cancer Lett.*, *99*: 93–97, 1996.

6. Dandona, P., Thusu, K., Cook, S., Snyder, B., Makowski, J., Armstrong, D., and Nicotera, T. Oxidative damage to DNA in diabetes mellitus. *Lancet*, *347*: 444–445, 1996.

7. Tagesson, C., Kallberg, M., Klintonberg, C., and Starkhammar, H. Determination of urinary 8-hydroxydeoxyguanosine by automated coupled-column high performance liquid chromatography: a powerful technique for assaying *in vivo* oxidative DNA damage in cancer patients. *Eur. J. Cancer*, *31A*: 934–940, 1995.

8. Loft, S., Vistisen, K., Ewertz, M., Tjonneland, A., Overvad, K., and Poulsen, H. E. Oxidative DNA damage estimated by 8-hydroxydeoxyguanosine excretion in humans: influence of smoking, gender and body mass index. *Carcinogenesis (Lond.)*, *13*: 2241–2247, 1992.

9. Shigenaga, M. K., Gimeno, C. J., and Ames, B. N. Urinary 8-hydroxy-2'-deoxyguanosine as a biological marker of *in vivo* oxidative DNA damage. *Proc. Natl. Acad. Sci. USA*, *86*: 9697–9701, 1989.

10. Ravanat, J.-L., Duret, B., Guiller, A., Duoki, T., and Cadet, J. Isotope dilution high-performance liquid chromatography-electrospray tandem mass spectrometry assay for the measurement of 8-oxo-7, 8-dihydro-2'-deoxyguanosine in biological samples. *J. Chromatogr. B*, *715*: 349–356, 1998.

11. Holmberg, I., Stal, P., and Hamberg, M. Quantitative determination of 8-hydroxy-2'-deoxyguanosine in human urine by isotope dilution mass spectrometry: normal levels in hemochromatosis. *Free Radic. Biol. Med.*, *26*: 129–135, 1999.

12. Witherell, H. L., Hiatt, R. A., Peplogle, M., and Parsonnet, J. *Helicobacter pylori* infection and urinary excretion of 8-hydroxy-2'-deoxyguanosine, an oxidative DNA adduct. *Cancer Epidemiol. Biomark. Prev.*, *7*: 91–96, 1998.

13. Toyokuni, S., Tanaka, T., Hattori, Y., Nishiyama, Y., Yoshida, A., Uchida, K., Hiai, H., Ochi, H., and Osawa, T. Quantitative immunohistochemical determination of 8-hydroxy-2'-deoxyguanosine by a monoclonal antibody N45.1: its application to ferric nitrilotriacetate-induced renal carcinogenesis model. *Lab. Investig.*, *76*: 365–374, 1997.

14. Erhola, M., Toyokuni, S., Okada, K., Tanaka, T., Hiai, H., Ochi, H., Uchida, K., Osawa, T., Nieminen, M. M., Alho, H., and Kellokumpu-Lehtinen, P. Biomarker evidence of DNA oxidation in lung cancer patients: association of urinary 8-hydroxy-2'-deoxyguanosine excretion with radiotherapy, chemotherapy, and response to treatment. *FEBS Lett.*, *409*: 287–291, 1997.

15. Prieme, H., Loft, S., Cutler, R. G., and Poulsen, H. E. Measurement of oxidative DNA injury in humans: evaluation of a commercially available ELISA assay. *In*: J. T. Kumpulainen and J. T. Salonen (eds.), *Natural Antioxidants and Food Quality in Atherosclerosis and Cancer Prevention*, pp. 78–82. London: The Royal Society of Chemistry, 1996.

16. Kasai, H., Iwamoto-Tanaka, N., Miyamoto, T., Kawanami, K., Kawanami, S., Kido, R., and Ikeda, M. Life style and urinary 8-hydroxydeoxyguanosine, a marker of oxidative DNA damage: effects of exercise, working conditions, meat intake, body mass index, and smoking. *Jpn. Cancer Res.*, *92*: 9–15, 2001.

17. Bogdanov, M. B., Beal, M. F., McCabe, D. R., Griffin, R. M., and Matson, W. R. A carbon column-based liquid chromatography electrochemical approach to routine 8-hydroxy-2'-deoxyguanosine measurements in urine and other biologic matrices: a one-year evaluation of methods. *Free Radic. Biol. Med.*, *27*: 647–666, 1999.

# Cancer Epidemiology, Biomarkers & Prevention

AACR American Association  
for Cancer Research

## Comparison between High-Performance Liquid Chromatography and Enzyme-linked Immunosorbent Assay for the Determination of 8-Hydroxy-2'-deoxyguanosine in Human Urine

Kayoko Shimoi, Hiroshi Kasai, Naoko Yokota, et al.

*Cancer Epidemiol Biomarkers Prev* 2002;11:767-770.

**Updated version** Access the most recent version of this article at:  
<http://cebp.aacrjournals.org/content/11/8/767>

**Cited articles** This article cites 14 articles, 3 of which you can access for free at:  
<http://cebp.aacrjournals.org/content/11/8/767.full#ref-list-1>

**Citing articles** This article has been cited by 5 HighWire-hosted articles. Access the articles at:  
<http://cebp.aacrjournals.org/content/11/8/767.full#related-urls>

**E-mail alerts** [Sign up to receive free email-alerts](#) related to this article or journal.

**Reprints and Subscriptions** To order reprints of this article or to subscribe to the journal, contact the AACR Publications Department at [pubs@aacr.org](mailto:pubs@aacr.org).

**Permissions** To request permission to re-use all or part of this article, use this link  
<http://cebp.aacrjournals.org/content/11/8/767>.  
Click on "Request Permissions" which will take you to the Copyright Clearance Center's (CCC) Rightslink site.